

ज्ञापांक 5706 / आपूर्ति

92-1-03/2017

पुलिस महानिदेशक का कार्यालय, बिहार, पटना।

पटना, दिनांक- 17-05-2017

सेवा में,

निदेशक,
सूचना एवं जनसम्पर्क विभाग,
बिहार, पटना।

विषय- निविदा आमंत्रण सूचना सं०-4/2017-18 के प्रकाशन के संबंध में।

निदेशानुसार उपर्युक्त विषय के संबंध में निविदा आमंत्रण सूचना सं०-4/2017-18 की पाँच प्रतियाँ (सी०डी० सहित) संलग्न करते हुए अनुरोध है कि इसे राज्य एवं राज्य से बाहर के प्रमुख समाचार पत्रों में (अंग्रेजी एवं हिन्दी) के अगले दो संस्करणों में प्रकाशित कराने की कृपा की जाय साथ ही पी०आर०डी० वेबसाइट पर भी प्रसारित करने की कृपा की जाय।

इस निविदा आमंत्रण सूचना का प्रकाशन किन-किन समाचार पत्रों में किया गया इसकी सूचना देने की कृपा की जाय।

अनु०-यथोपरि।

16/5
पुलिस महानिरीक्षक के सहायक (क्यू०),
बिहार, पटना।

प्रतिलिपि:-

1. आई०टी० मैनेजर, पुलिस महानिदेशक का कार्यालय, बिहार, पटना को कृपया सूचनार्थ। कृपया इसे आज ही वेबसाइट पर अपलोड किया जाय। साथ ही Indian Trade Journal, Kolkata के अंक में प्रकाशन हेतु Government of India, the Controller of Publications, Civil Lines, Delhi : 110 054, (Tel No. 011-23812527, FAX : 011-23817846), Email Id-sk.mondal.dgcis@nic.in के पते पर भी अनिवार्य रूप से भेजा जाय।
2. Government of India, the Controller of Publications, Civil Lines, Delhi : 110 054, (Tel No. 011-23812527, FAX : 011-23817846), Email Id- sk.mondal.dgcis@nic.in को कृपया सूचनार्थ एवं आवश्यक क्रियार्थ प्रेषित। अनुरोध है कि उक्त निविदा का प्रकाशन Indian Trade Journal, Kolkata के अंक में करने की कृपा की जाय।

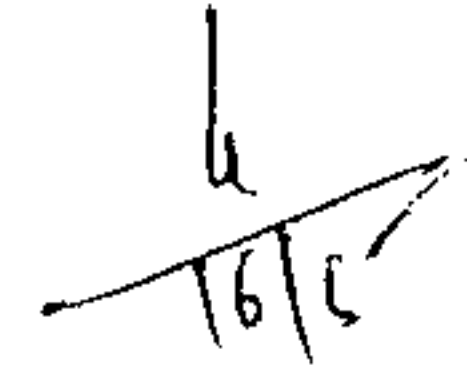
16/5
पुलिस महानिरीक्षक के सहायक (क्यू०),
बिहार, पटना।

Police Headquarters, Bihar, Patna
Notice Inviting Tender No. 4/2017-18

1. Name of the Department : Office of Director General of Police, Bihar, Patna.
2. Last date & time for the acceptance of the tender : 19 / 6 /2017, Till 11:00 AM
3. Date & time fixed for the opening of the tender : 19 / 6 /2017 At 11:15 AM
4. Place fixed for receiving & opening the tender : Office of Director General of Police, Bihar, Patna.
5. Details of Job :

S.N.	Item name	Quantity
1.	Stereo Microscope	01
2.	Bullet Recovery Box	02
3.	UV Lamp	02
4.	Hot Air Oven	02
5.	Deep Freezer	02
6.	Crime Scene Investigation Kit	06

Specifications and other terms & conditions of the tender may be obtained in person from this office or may be downloaded from the website www.prdbihar.gov.in or www.biharpolice.bih.nic.in.

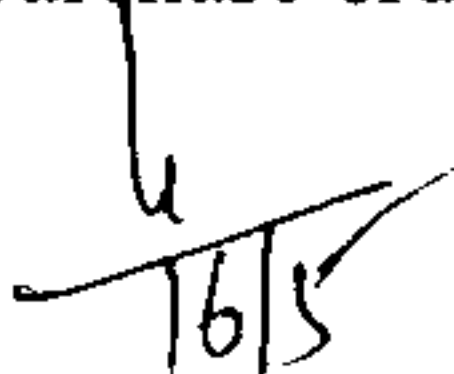


AIG (Q)
Bihar, Patna

Terms & Conditions Of Tender No. 4/2017-18

1. Tender of the firm will be accepted only on the condition that if their tenders are approved, the firm shall get registered with the Commercial Tax Department, Bihar, before the purchase order is issued.
2. The tender should be submitted in two parts : (i) Technical Bid and (ii) Financial Bid, duly sealed in two separate envelopes super-scribed as "Technical Bid" and "Financial Bid".
3. All relevant papers/ E.M.D./certificates/specifications etc. of items should be enclosed in the Technical Bid.
4. The rates of the items shall be quoted in the Financial Bid only.
5. All charges like BST/CST/Service Tax /VAT etc. shall be clearly mentioned in the Financial Bid and the net rate (in figures and words) including all taxes and duties must also be quoted. Vague offers like indicating taxes "as applicable" will not be accepted.
6. The rates of the items shall be quoted in the Financial Bid in two parts :
(i) With AMC (Annual Maintenance Contract) and (ii) Without AMC
7. There should be no cutting, over writing or correction on the rates.
8. The technical and financial bids for each item should be submitted separately in separate envelopes. The technical and financial bids for more than one items submitted together in the same envelope shall not be accepted.
9. If the financial bid is submitted in the same envelope containing the technical bid then also it shall be summarily rejected.
10. The technical and financial bids should be put in two separate sealed envelopes and the envelopes should be marked Tender No-4/2017-18 (Technical Bid) and Tender No-4/2017-18 (Financial Bid) along with the name and address of the firm. The sealed envelopes containing the technical and the financial bids should be sent in another sealed envelope which should be marked as Tender No-4/2017-18. This envelope should not bear the name and address of the firm.
11. Income Tax Returns of last three years, a photocopy of PAN of the participating firm and turn-over of any two of the previous three financial years should be submitted with the technical bid. It should be specifically mentioned whether IT return has been filed manually or electronically.
12. The turn over of the firm for the last reported financial year should be at least double the amount of the supply order which is being issued. A copy of the profit and loss Account of the firm for any two of the previous three financial years, certified by a Chartered Accountant should be submitted along with the tender. If the tenderer is authorized dealer or authorized supplier of manufacturing firm, then the certified details of the turnover of authorizing firm may be accepted. Tender specific authorization from the OEM must be submitted, but in certain cases where authorization from OEM is not required, the Technical-cum-User committee (T.U.C.) shall decide about exemption (if any) on a case-by-case basis; citing appropriate reasons for the same.
13. If there is some discount in the price of any item, it should be deducted from price itself and such discounts should not be quoted separately.
14. If the product is available on DGS & D rate contract, then a copy of the contract must be attached and pricing be done including all taxes.

15. A copy of the test report for the product issued by any established and recognized private Laboratory or by agency accredited by the Government should be attached with the technical bid. However if required, the Technical-cum-User committee (T.U.C.) can take decision regarding exemptions/relaxations (if any), citing appropriate reasons.
16. In case of Bullet Proof/Bullet Resistant items, test report of TBRL is compulsory.
17. Firms participating in this tender shall also submit duly sworn affidavit to the effect that " this firm has not been black listed/debarred by any Government or Semi Government or Private Agency and no sister concern of this firm is participating in this tender."
18. Firms participating in this tender shall also submit the self attested list of users of its equipments.
19. All items shall be received at Central Clothing Store, Patna, therefore price should be quoted FOR Central Clothing Store, Phulwari Sharif, Patna.
20. Firms will have to deposit a sum of Rs.50,000/- (Fifty Thousand) only as an earnest money deposit in the form of Bank Draft duly pledged in favour of the undersigned along with the quotations. The small scale units located in Bihar shall not be liable to deposit earnest money. Exemption from submitting E.M.D. will also be available to those who are registered with the Central Purchase Organisation/State Purchase Organisation and National Small Industries Corporation (NSIC).
21. Technical Bids will be opened on scheduled date and time in the office chamber of Police Headquarter. Representatives of the firms competing in the tender may remain present at the time of opening of the technical bid.
22. The technical bids will be opened first and placed before the Technical Committee of the Police Headquarters, Bihar. If the technical bids are found satisfactory as per tender conditions, it will be put before Central Purchase Committee of the Police Headquarters, Bihar. The firms may be required to participate in the demonstrations of the quoted product and discussions with this committee.
23. Any paper/document will not be accepted after opening the tender.
24. Successful firm will have to enter into an agreement after depositing a sum of 5% of the total value of the order as security money in the form of Bank Guarantee duly pledged in favor of undersigned.
25. The firm will be required to provide satisfactory after-sales service after the delivery of the product.
26. The firm will be required to supply all the items within the stipulated time frame as mentioned in the purchase order.
27. Payment for the delivered items will be made only after the acceptance report of the Inspection Committee of the Police Headquarters, Bihar.
28. The firm whose quotation is approved by the Central Purchase Committee of the Police Headquarters, Bihar, shall be invited to enter into an agreement with the undersigned.
29. It is expected to submit the duly filled chart attached herewith, along with the technical bid.
30. Indexing of the requisite documents must be done and submitted along with the technical bid.
31. Hands on training of the equipment must be imparted to the user group by the firm.
32. Director General of Police Bihar, Patna reserves the right to reject any or all the quotations partially or fully, without assigning any reason thereof.
33. The Quantity indicated may increase or decrease at the time of issuing purchase order.


A I G (Q)
Bihar, Police.

13
27
50
25

Bullet recovery box with lid
Specification

- (i) Made of wood.
- (ii) Dimension – 20 ft x 1.5 ft. x 1.5 ft.
- (iii) Internal side quoted with 16 gauze iron sheet
- (iv) Internal side contain block of length 2ft
- (v) With lid.
- (vi) One front side open and other side closed.
- (vii) Filled with cotton.

Crime scene investigation kit.

- (i) 05 mtr tape measure – 1
- (ii) Flash light – 1
- (iii) Big rolls of evidence tape – 02.
- (iv) Small rolls of evidence tape – 02
- (v) Evidence labels – 20
- (vi) Evidence tags with ties – 20
- (vii) Chain of possession labels – 20
- (viii) Portable ultraviolet light with batteries – 01
- (ix) Assorted evidence collection litters – 20
- (x) Twizzers – 02
- (xi) Pair of scissors – 01
- (xii) Scriber – 01
- (xiii) Swiss knife 21 function – 01
- (xiv) Marker, Black & white – 01
- (xv) Liquid sampling pipettes – 04
- (xvi) 3" magnifying glass – 01
- (xvii) Probe with paint chip cutter – 01
- (xviii) Sticks of white chalk – 03
- (xix) Collection tubes with EDTA- 12
- (xx) Disposable syringes – 02
- (xxi) Plastic containers with caps – 03
- (xxii) Disposable latex glove caps – 03
- (xxiii) Stainless steel spatula – 01
- (xxiv) Disposable scalpel – 01
- (xxv) Steel measuring tape – 01
- (xxvi) Inkless round finger print pad with elimination slips – 01
- (xxvii) Inner storage case – 01
- (xxviii) Molded/Aluminium carrying case with metal from - 01
- (xxix) Benzedrine and H₂O₂ soln. – 05 (each)
- (xxx) Mask (disposable)

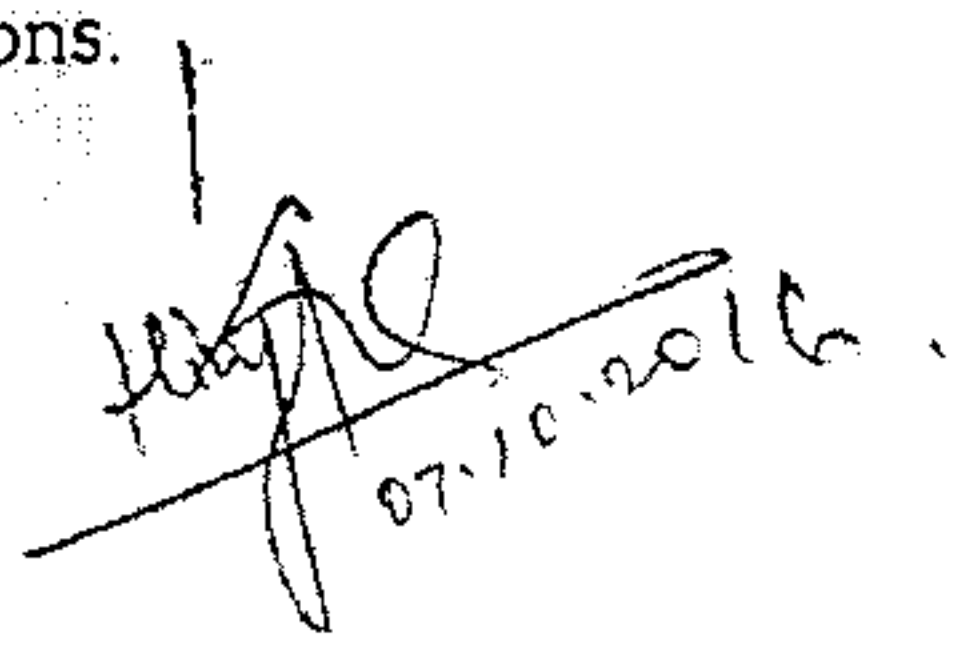
Stb
07/10/86

12
26
30

HOT AIR OVEN

TECHNICAL SPECIFICATIONS

1. Should be operated on 230V, 50Hz single phase AC supply and having temperature ranging between 50-200°C
2. Should be made of double walled chamber -Inner made of stainless steel SS 304 grade and powder coated outer surface.
3. Should provide with three heating elements on three sides of the equipment for uniform temperature on all shelves.
4. Should be provided with air circulating fan.
5. Should provide with a variable microprocessor based digital temperature controller with digital display and thermometer should be provided separate.
6. Should have a minimum chamber size of (L*B*H) 450*450*450 with 2 stainless steel trays with holes.
7. Should provide with air ventilations.


07.10.2016

11
25
30
27

CHROMATOGRAPHY VISUALISATION : UV LAMP

UV Lamp, Model 4 (Jan. 2016) Dual wavelength 254 nm + 366 nm with guaranteed minimum intensity, as follows : UV lamp at 17 cm distance. Short wave UV (254 nm) 1600, long wave (366 nm) 1000. Visible light (<400nm) 0.4. Full protection to viewer's eyes and skin from UV light for safety. High tech 50 kHz power supply for flickerless, instant illumination. Auto switch off after 10 min. Thermal sensor and tilt sensor built in for user safety.

Essential Accessories

1. Guarantee- one year
2. Comprehensive warranty for entire system next 2 years
3. Non comprehensive AMC for next 3 years. Please provide year wise AMC offer.
4. CMC for next 2 years, please provide year wise CMC offer(including service charges or any other taxes if applicable).
5. Complete operational trainings to be provided to working analysts at site.
6. All related and essential accessories are to be quoted.
7. At least 10 day's onsite training after installation should be provided.
8. Spare parts for two years/Requisite must be supplied with the system for smooth operation.
9. Installation, commissioning at the end user site - free of cost.

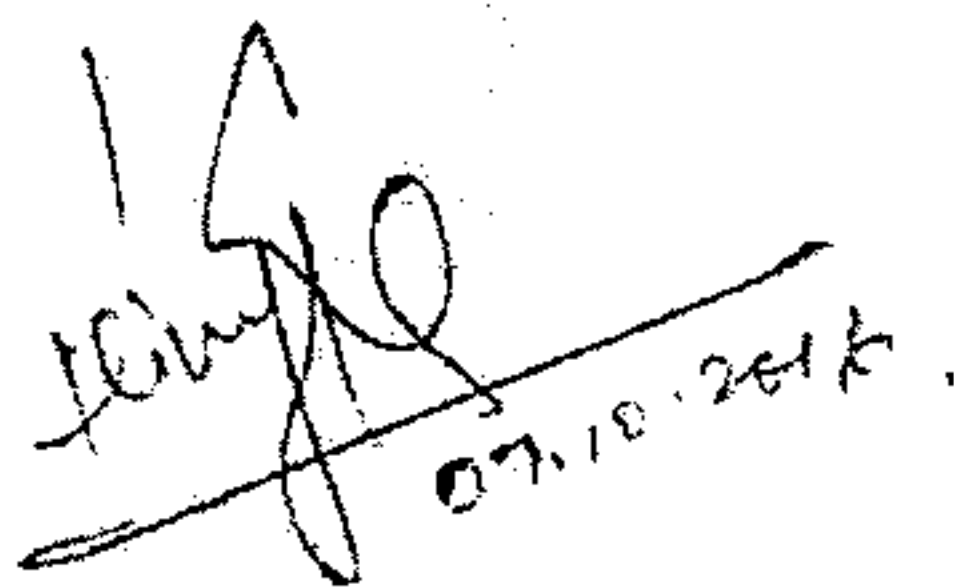
dm

*Perla
29.05.16*

10
24
24
28

"Specification for Deep Freezer"

- Deep freezer is a low temperature freezer with range of -20deg C with temperature deviation of ± 3 deg C.
- Interior cabinet made of Stainless steel.
- Exterior made of durable non-corrosive powder coated galvanised steel.
- Stainless steel adjustable shelves and compartments provide with separate inner poly-acrylic sub-doors.
- High Density PUF insulation of 75 mm thickness for the cabinet.
- PUF insulated, left hinged, main door with inner FRP lining and lock.
- Hot line around the front of the cabinet to prevent moisture condensation.
- Equipment mounted on lockable castor wheels.
- Silent energy efficient refrigeration system with hermetically sealed compressor and CFC and HCFC free eco-friendly refrigerant.
- Specially designed air-cooled condenser to ensure that the equipment occupies very less space.
- Air cooled condensation system, aided by continuous rated motor fans
- Main door with heavy duty latch and magnetic rubber gasket ensures tight closure
- Refrigeration system with overload protectors and MCB
- Microprocessor based temperature control system with audio visual alarm for high/low temperature deviation.
- Thermistor sensor for accurate temperature measurement.
- Temperature calibration traceable to National Standards.
- Automatic Voltage stabilizer with time delay restart
- CE marked
- Temperature Chart recorder, Cryo Coolant Cassettes back-up, inventory system (Cryo racks & Cryo boxes) etc.
- Compete with latest Model
- Capacity :- 380 Litre
- Dimension- Inner Chamber 1000x620x610 mm.
- Including all accessories for installation.
- Warranty 03 years.


07.10.2015

498
9

STEREOMICROSCOPE SYSTEM SPECIFICATION AS PER THE REQUIREMENT IN REGIONAL FORENSIC LABORATORY, BIHAR

1. Optical System should be Galilean Optical System.
2. Coded/Motorized Zoom with zooming ratio 20:5:1.
3. Observation Tube should be Trinocular/Tilting Trinocular Observation Tube and beampath switchable camera or eyepiece.
4. Standard Magnification of 7.8x to 160x.
5. Optical Resolution to be approximately 0.952 μ m.
6. Software with live measurement of the features such as radius, angle, diameter, distance from defined length, centre to centre distance between two circles.
7. Incident illumination, Ring Light illumination and double flexible light guide with LED Source.
8. A table top stand-alone controller for display of all microscopic coded parameters cum controller for motorized focus.
9. C-mount Digital colour camera with Dynamic range 900:1dB, pixel size 3.4 μ m*3.4 μ m and resolution 5 megapixel CCD sensor.
10. Competent with latest model.

Specification for Trinocular Microscope

1. Achromatic objective – 5x, 10x, 45x and 100x
2. Eye piece – 10x, 15x
3. Magnification – 50x – 1500x
4. Oil immersion, detachable mechanical stage.
5. Computer Compatible software.
6. Branded Computer with colour printer.

HPLC Specification

The HPLC System analyze the forensic compounds, toxicological compound, Explosive material etc.

Quaternary Gradient Pump (4 solvents) with degasser minimum four channel or higher.

Flow rate 0.01-10ml/min or better.

System back pressure of minimum 8000 psi or better.

Flow rate accuracy \pm 0.1% or better

Flow precision of \leq 0.075% RSD or better.

Solvent rack and solvent bottles (at least four) also to be quoted

Auto sampler:-

Thermostated auto-sampler: Temperature range 4^o.40^o or better.

With minimum 300 injection vials and injection volume range of up to (1-100 μ L).

Programmable needle with wash/purge option to minimize carryover. Needle wash internal and External.

498
16/6/16

498